


Access is an aspheric lens that provides near and intermediate vision correction for presbyopes.

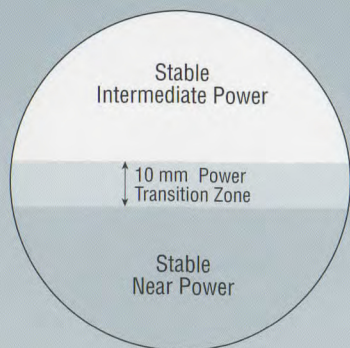

## Fitting Access

### 1 Frame Selection

For best vision and appearance, encourage the patient to choose a frame in which the eyes are well centered with a minimum "B" of 30 mm. Ideally, the pupils should fall within 5 mm of the frame's vertical center.

### 2 Frame Adjustment


The frame must be adjusted correctly prior to taking any measurements. Ensure the following:

- 10° to 12° pantoscopic tilt.
- Proper face form wrap.
- Close frame fit (i.e., short vertex distance), without touching skin or eyelashes.



### 3 Fitting Height

Check that the patient's pupils fall within 5 mm of the vertical center of the frame. If not, decenter the lens vertically as needed.

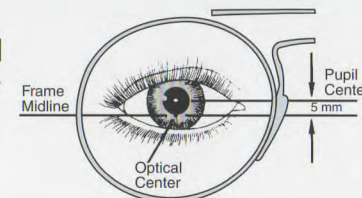

### 4 Pupillary Distance

Since Access will be used for near and intermediate range viewing, measure the **near PD** with a pupillometer or PD ruler. Monocular PDs are not necessary.

### 5 Lens Selection

Your laboratory will use the criteria below to select the appropriate lens for your patient's Rx (unless you specify otherwise):

- Low power range (0.75 Diopter) for presbyopes with a +1.50 add or less.
- High power range (1.25 Diopter) for presbyopes with a +1.75 add or greater.

## Verifying Cut-Out

- 1 Place the frame down with the right lens over the chart.
- 2 Move the frame until the center of the bridge is at the required near PD.
- 3 Position the frame up or down until it is centered vertically.
- 4 If the lens area of the frame falls within the circle, then the selected frame will work.



## Questions?

Call SOLA  
Technical Services Hotline


**1-800-358-8258**

press 3



## Base Curve Selection Chart

Near Rx Power

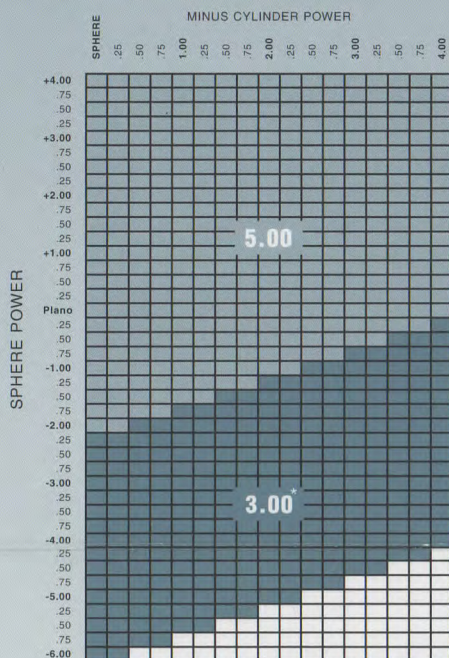

\*Hard resin only. Please confirm availability.

**ACCESS<sup>®</sup>** The lens for today's  
computer workplace

**SOLA**  
OPTICAL USA

2277 PINE VIEW WAY  
PETALUMA, CA 94954


## Verifying Access

### 1 Reading Rx

Verify the lens for the correct **reading** Rx below the dashed arc. Verify the Rx axis when the 180° line of the lens is horizontal.

### 2 Verify Prism

Check the lens for prescribed prism or prism imbalance at the Prism Reference Point (PRP) in the center of the lens.

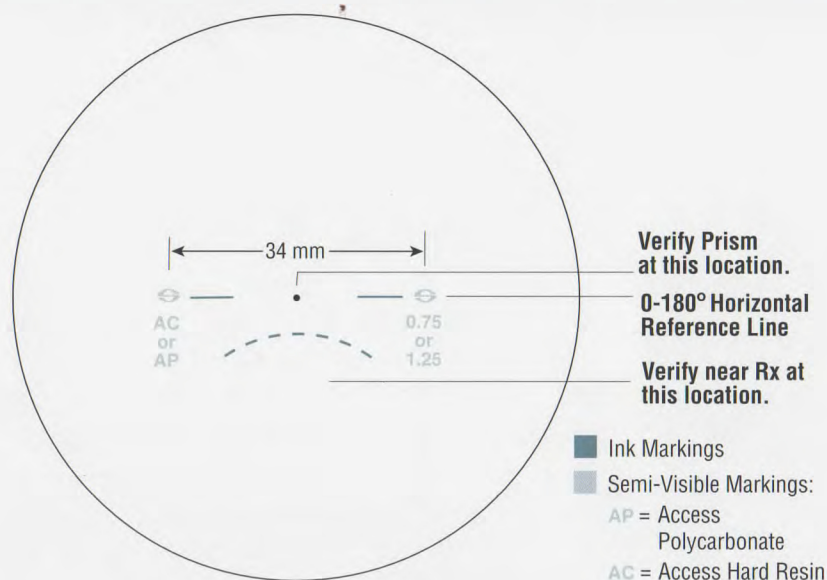

## Dispensing Access


### 1 Frame Alignment

Fine tune the adjustment and alignment of the frame to correct any changes that may have occurred during lens insertion and handling.

### 2 Patient Instruction

Instruct the patient on the proper use and handling of Access lenses.

Remind the patient to wear Access **only for stationary activities** – not for walking or driving.

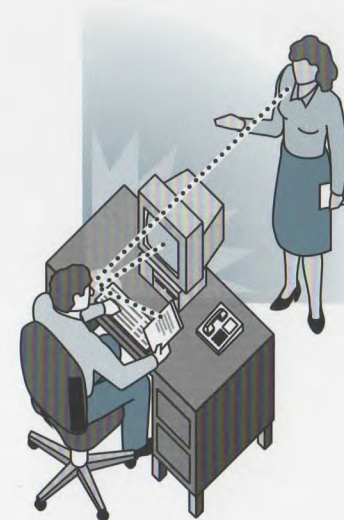

Access lenses provide a clear view of the computer work area and beyond — up to seven feet.